


Medtronic

Engineering the extraordinary


Aortic product catalog



Endurant™ II/IIIs Stent Graft System



Valiant™ Stent Graft with Captivia™ Delivery System




Heli-FX™ EndoAnchor™ System



Steerant™ Super Stiff Guidewire



Sentrant™ Introducer Sheath with Hydrophilic Coating



Reliant™ Stent-Graft Balloon Catheter

Table of contents

- 03 **Endurant™ II/IIIs**
Stent Graft System
- 27 **Valiant™ Stent Graft**
with Captivia™ Delivery System
- 41 **Heli-FX™**
EndoAnchor™ System
- 43 **Steerant™**
Super Stiff Guidewire
- 45 **Sentrant™**
Introducer Sheath with Hydrophilic Coating
- 47 **Reliant™**
Stent-Graft Balloon Catheter

Endurant™ II/IIIs

Stent Graft System

Features†

You can be confident in your outcomes with a design that addresses sac regression.

Accurate placement & controlled deployment

- Intuitive graft deployment system provides controlled release of the suprarenal stent & anchor pins and offers controlled delivery at the intended target zone with 99.1% delivery and deployment success (ENGAGE PAS¹)
- Tip capture deployment mechanism allows precise positioning – even after deployment of 3 stent rings– and allows greater control of deployment and landing accuracy

Continuous seal, fixation & graft comfortability

- M-shaped proximal stents maximize wall apposition & circumferential conformability and minimize in-folding resulting in low Type Ia endoleak rates
- 45° suprarenal stent anchor pins provide secure fixation over time and reduce main migration risk and device movement
- Electropolished nitinol stent maximize circumferential conformability with dynamic continuous seal


Durable hemostatic barrier & resistance against type II ELs

- Graft material addresses sac regression provides durable hemostatic barrier and reduced Type II endoleaks
- Multifilament polyester material provides low permeability

† Test data on file at Medtronic. Bench test results may not be indicative of clinical performance.

¹ Endurant Stent Graft System Post Approval Study (ENGAGE PAS), Duke Clinical Research Institute, Last update posted October 29, 2021, <https://classic.clinicaltrials.gov/ct2/show/NCT01379222>

Optimize
outcomes for
the broadest
patient base

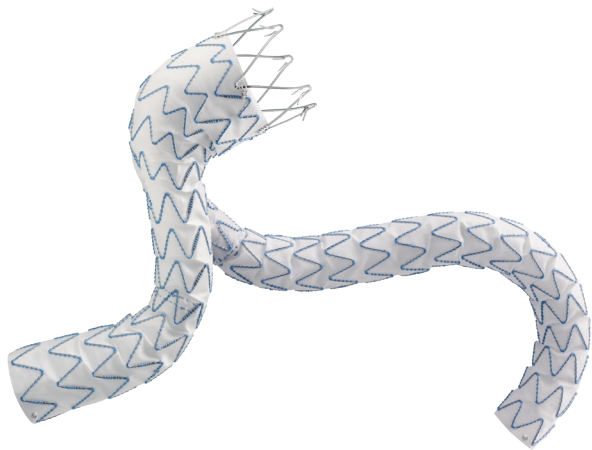


Endurant™ II/IIs

Stent Graft System

Endurant™ II/IIs system product code description

ET	B	F	23	13	C	124	EE	18
								Catheter outer diameter
							Delivery system	EE - Endurant™ II system
						Total covered length		
					Distal design	C - Closed web		
				Distal graft diameter				
			Proximal graft diameter					
		Proximal design	F - FreeFlo W - Open web					
		Device configuration	B - Bifurcations L - Limbs E - Iliac extension C - Extensions & cuffs T - Extensions & cuffs U - Aorto-uni-iliac (AUI)					
		Product name	ET - Endurant™ II system ES - Endurant™ IIs system					

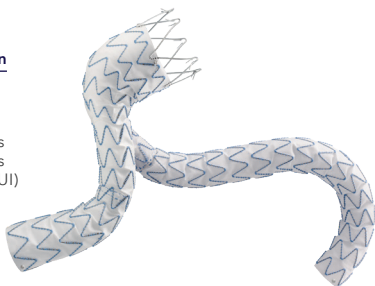

Endurant™ IIs system bifurcations

Product code						
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system	Catheter outer diameter (Fr)
ESBF	23	14	C	103	EE	18
ESBF	25	14	C	103	EE	18
ESBF	28	14	C	103	EE	18
ESBF	32	14	C	103	EE	20
ESBF	36	14	C	103	EE	20



Endurant™ II system bifurcations

Product code						
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system	Catheter outer diameter (Fr)
ETBF	23	13	C	124	EE	18
ETBF	23	13	C	145	EE	18
ETBF	23	13	C	166	EE	18
ETBF	23	16	C	124	EE	18
ETBF	23	16	C	145	EE	18
ETBF	23	16	C	166	EE	18
ETBF	25	13	C	124	EE	18
ETBF	25	13	C	145	EE	18
ETBF	25	13	C	166	EE	18
ETBF	25	16	C	124	EE	18
ETBF	25	16	C	145	EE	18
ETBF	25	16	C	166	EE	18
ETBF	28	13	C	124	EE	18
ETBF	28	13	C	145	EE	18
ETBF	28	13	C	166	EE	18
ETBF	28	16	C	124	EE	18
ETBF	28	16	C	145	EE	18
ETBF	28	16	C	166	EE	18
ETBF	28	20	C	124	EE	18
ETBF	28	20	C	145	EE	18
ETBF	28	20	C	166	EE	18
ETBF	32	16	C	124	EE	20
ETBF	32	16	C	145	EE	20
ETBF	32	16	C	166	EE	20
ETBF	32	20	C	124	EE	20
ETBF	32	20	C	145	EE	20
ETBF	32	20	C	166	EE	20
ETBF	36	16	C	145	EE	20
ETBF	36	16	C	166	EE	20
ETBF	36	20	C	145	EE	20
ETBF	36	20	C	166	EE	20

Endurant™ II/IIs

Stent Graft System

Limbs†

	Product code					Catheter outer diameter (Fr)	Total contralateral covered length with EII/EIIs bifurcated**	Total ipsilateral covered length with EIIs bifurcated††
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system			
ETLW	16	10	C	82	EE	14	132	152
ETLW	16	10	C	93	EE	14	143	163
ETLW	16	10	C	124	EE	14	174	174 - 194
ETLW	16	10	C	146	EE	16	196	196 - 216
ETLW	16	10	C	156	EE	16	206	206 - 226
ETLW	16	10	C	199	EE	16	249	249 - 269
ETLW	16	13	C	82	EE	14	132	152
ETLW	16	13	C	93	EE	14	143	163
ETLW	16	13	C	124	EE	14	174	174 - 194
ETLW	16	13	C	146	EE	16	196	196 - 216
ETLW	16	13	C	156	EE	16	206	206 - 226
ETLW	16	13	C	199	EE	16	249	249 - 269
ETLW	16	16	C	82	EE	14	132	132 - 152
ETLW	16	16	C	93	EE	14	143	143 - 163
ETLW	16	16	C	124	EE	14	174	174 - 194
ETLW	16	16	C	146	EE	16	196	196 - 216
ETLW	16	16	C	156	EE	16	206	206 - 226
ETLW	16	16	C	199	EE	16	249	249 - 269
ETLW	16	20	C	82	EE	16	132	152
ETLW	16	20	C	93	EE	16	143	163
ETLW	16	20	C	124	EE	16	174	174 - 194
ETLW	16	20	C	146	EE	16	196	196 - 216
ETLW	16	20	C	156	EE	16	206	206 - 226
ETLW	16	20	C	199	EE	16	249	249 - 269
ETLW	16	24	C	82	EE	16	132	152
ETLW	16	24	C	93	EE	16	143	163
ETLW	16	24	C	124	EE	16	174	174 - 194
ETLW	16	24	C	146	EE	16	196	196 - 216
ETLW	16	24	C	156	EE	16	206	206 - 226
ETLW	16	24	C	199	EE	16	249	249 - 269
ETLW	16	28	C	82	EE	16	132	152
ETLW	16	28	C	93	EE	16	143	163
ETLW	16	28	C	124	EE	16	174	174 - 194
ETLW	16	28	C	146	EE	16	196	196 - 216
ETLW	16	28	C	156	EE	16	206	206 - 226
ETLW	16	28	C	199	EE	16	249	249 - 269

† The limb mates with the AUI stent graft on the ipsilateral side.

** These calculations assume the minimum 30 mm overlap between the bifurcated stent graft and the contralateral iliac limb per the Endurant™ II stent graft system *Instructions for Use*. When using the 124 mm length bifurcated stent graft, subtract 10 mm from total contralateral covered length with bifurcated.

†† The 3-5 stent overlap is available only with select limbs. Please refer to the *Instructions for Use* for more information.

Some products, /indications/therapy areas may not be licensed in accordance with Canadian Law.



Iliac extensions

Product code						
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system	Catheter outer diameter (Fr)
ETEW	10	10	C	82	EE	14
ETEW	13	13	C	82	EE	14
ETEW	20	20	C	82	EE	16
ETEW	24	24	C	82	EE	16
ETEW	28	28	C	82	EE	18

Aortic extensions

Product code						
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system	Catheter outer diameter (Fr)
ETCF	23	23	C	49	EE	18
ETCF	25	25	C	49	EE	18
ETCF	28	28	C	49	EE	18
ETCF	32	32	C	49	EE	20
ETCF	36	36	C	49	EE	20
ETTF	23	23	C	70	EE	18
ETTF	25	25	C	70	EE	18
ETTF	28	28	C	70	EE	18
ETTF	32	32	C	70	EE	20
ETTF	36	36	C	70	EE	20

AUI

Product code						
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system	Catheter outer diameter (Fr)
ETUF	23	14	C	102	EE	18
ETUF	25	14	C	102	EE	18
ETUF	28	14	C	102	EE	18
ETUF	32	14	C	102	EE	20
ETUF	36	14	C	102	EE	20


Endurant™ II/IIs

Stent Graft System

Placement and sizing guidelines

Use the proximal radiopaque markers to position the top edge of the graft material.

e e-shaped marker assists with A/P orientation

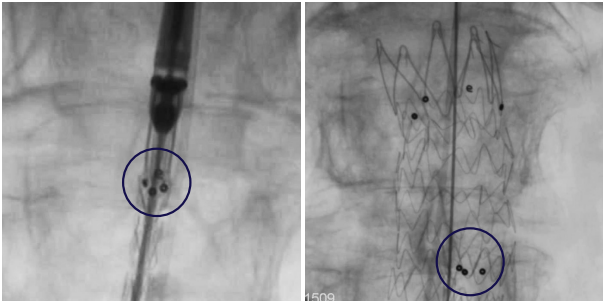

Radiopaque markers

For the contralateral side: The radiopaque markers at the proximal limb should be aligned with the radiopaque markers at the flow divider of the Endurant™ II system or Endurant™ II's system bifurs.

For the ipsilateral side: Depending on the limb configuration used, the radiopaque markers at the proximal end of the limb should be aligned to the distal radiopaque marker on the ipsilateral leg or the flow divider marker of the Endurant™ II's system bifur. Select limbs will allow a 3-5 stent overlap adjustment during the case. Please refer to the *Instructions for Use* for more information as needed.



Each Endurant™ II/Endurant™ IIs AAA stent graft must be ordered in a size that is appropriate to fit the patient's anatomy. Proper sizing of the Endurant™ II/Endurant™ IIs AAA stent graft is the responsibility of the physician. The following suggestions for stent graft diameters are based on vessel **inner wall** measurements.

Bifurcations, AUI and aortic extensions

Native vessel (mm)	Recommended Endurant™ II system diameter (mm)
19-20	23
21-22	25
23-25	28
26-28	32
29-32	36

Iliac extensions

Native vessel (mm)	Recommended Endurant™ II system diameter (mm)
8-9	10
10-11	13
15-18	20
19-22	24
23-25	28

Limbs


Native vessel (mm)	Recommended Endurant™ II system diameter (mm)
8-9	10
10-11	13
12-14	16
15-18	20
19-22	24
23-25	28

Endurant™ II/IIs

Stent Graft System

Component placement guide†

Endurant™ II system

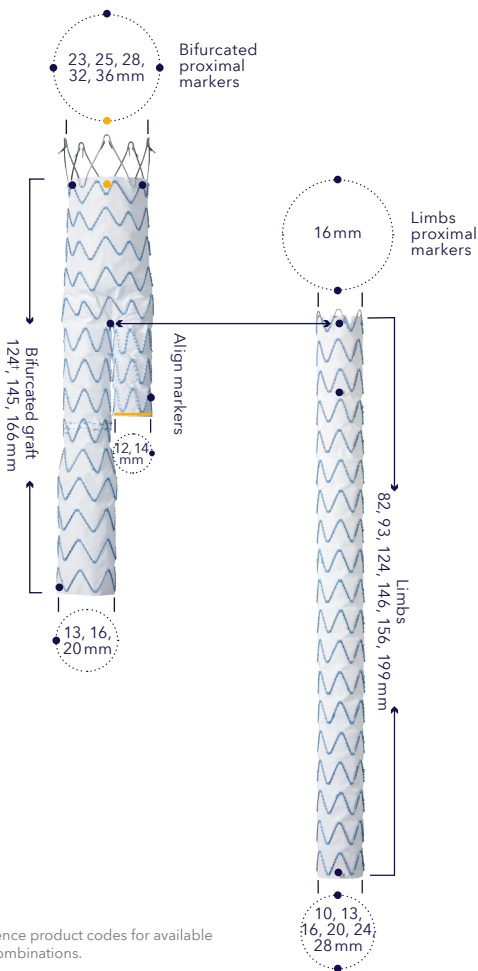


† Reference product codes for available size combinations.

Endurant™ II/IIs



Stent Graft System

Component placement guide

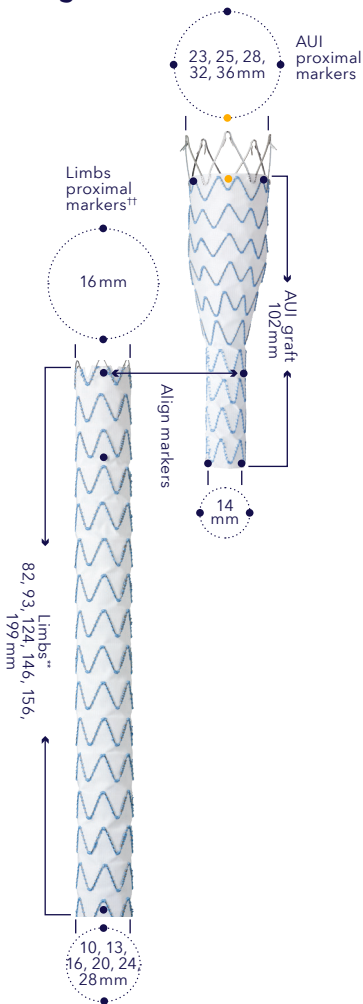

^{**} The limb mates with the Endurant™ II AUI stent graft on the ipsilateral side.

^{††} Requires minimum 3 stent overlap. See *Instructions for Use* for more information.

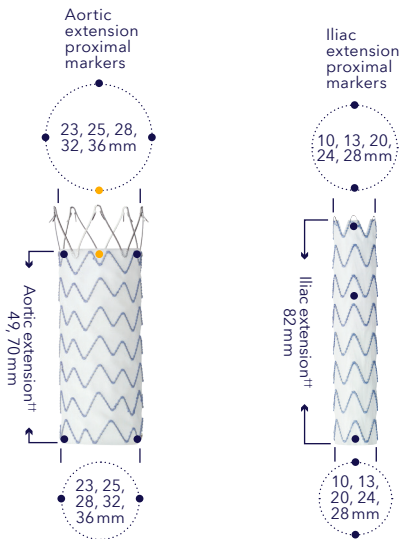


Distinct radiopaque markers

- Radiopaque markers
- e-shaped proximal markers

†† Requires minimum 3 stent overlap. See *Instructions for Use* for more information.

Endurant™ II/IIs

Stent Graft System

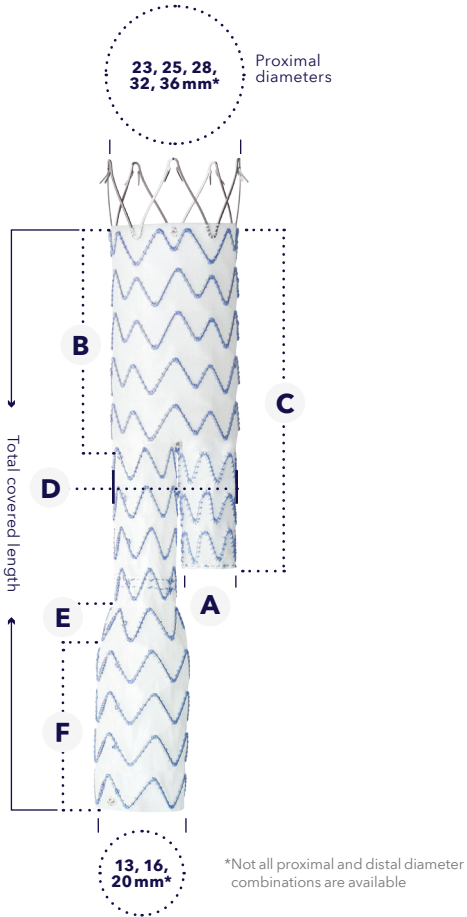

Endurant™ II system bifurcations




Endurant™ II system bifurcations


	Product code					Graft dimensions (mm)					
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system	A	B	C	D	E	F
	ETBF	23	13	C	124	EE	12	40	74	25	-
ETBF	23	13	C	145	EE	12	50	84	25	-	-
ETBF	23	13	C	166	EE	12	50	84	25	-	-
ETBF	23	16	C	124	EE	12	40	74	25	10	30
ETBF	23	16	C	145	EE	12	50	84	25	10	40
ETBF	23	16	C	166	EE	12	50	84	25	10	60
ETBF	25	13	C	124	EE	14	40	74	27	-	-
ETBF	25	13	C	145	EE	14	50	84	27	-	-
ETBF	25	13	C	166	EE	14	50	84	27	-	-
ETBF	25	16	C	124	EE	14	40	74	30	-	-
ETBF	25	16	C	145	EE	14	50	84	30	-	-
ETBF	25	16	C	166	EE	14	50	84	30	-	-
ETBF	28	13	C	124	EE	14	40	74	27	-	-
ETBF	28	13	C	145	EE	14	50	84	27	-	-
ETBF	28	13	C	166	EE	14	50	84	27	-	-
ETBF	28	16	C	124	EE	14	40	74	30	-	-
ETBF	28	16	C	145	EE	14	50	84	30	-	-
ETBF	28	16	C	166	EE	14	50	84	30	-	-
ETBF	28	20	C	124	EE	14	40	74	30	10	30
ETBF	28	20	C	145	EE	14	50	84	30	10	40
ETBF	28	20	C	166	EE	14	50	84	30	10	60
ETBF	32	16	C	124	EE	14	40	74	30	-	-
ETBF	32	16	C	145	EE	14	50	84	30	-	-
ETBF	32	16	C	166	EE	14	50	84	30	-	-
ETBF	32	20	C	124	EE	14	40	74	30	10	30
ETBF	32	20	C	145	EE	14	50	84	30	10	40
ETBF	32	20	C	166	EE	14	50	84	30	10	60
ETBF	36	16	C	145	EE	14	50	84	30	-	-
ETBF	36	16	C	166	EE	14	50	84	30	-	-
ETBF	36	20	C	145	EE	14	50	84	30	10	40
ETBF	36	20	C	166	EE	14	50	84	30	10	60

Endurant™ II/IIs

Stent Graft System

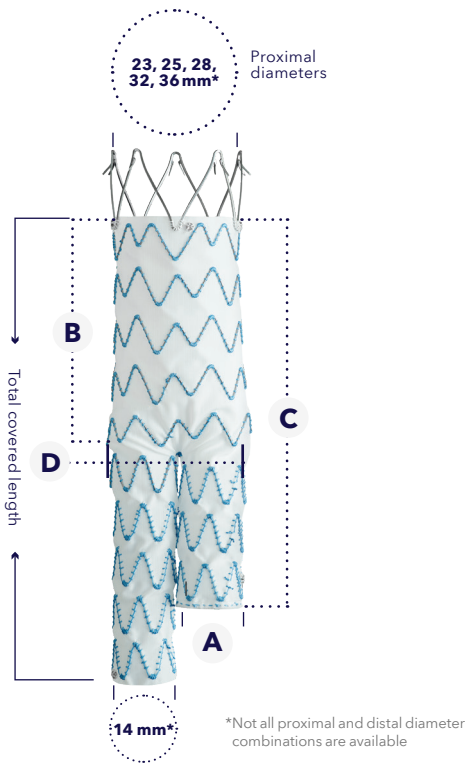

Endurant™ IIs system bifurcations



Endurant™ IIs system bifurcations


	Product code					Graft dimensions (mm)			
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system	A	B	C	D
ESBF	23	14	C	103	EE	14	50	84	28
ESBF	25	14	C	103	EE	14	50	84	28
ESBF	28	14	C	103	EE	14	50	84	28
ESBF	32	14	C	103	EE	14	50	84	28
ESBF	36	14	C	103	EE	14	50	84	28

Endurant™ II/IIs


Stent Graft System

Tapered limbs

	Product code					Graft dimensions (mm)	
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system	A	B
ETLW	16	10	C	82	EE	20	30
ETLW	16	10	C	93	EE	20	40
ETLW	16	10	C	124	EE	20	40
ETLW	16	10	C	156	EE	20	72
ETLW	16	10	C	199	EE	20	115
ETLW	16	13	C	82	EE	10	30
ETLW	16	13	C	93	EE	10	40
ETLW	16	13	C	124	EE	10	40
ETLW	16	13	C	156	EE	10	72
ETLW	16	13	C	199	EE	10	115

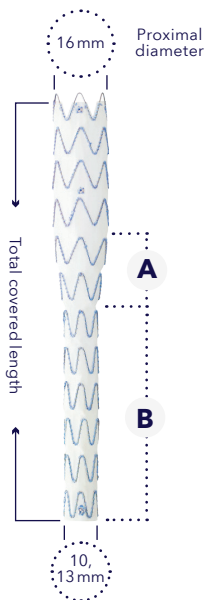


Tapered limbs



Straight limbs


Product code					
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system
ETLW	16	16	C	82	EE
ETLW	16	16	C	93	EE
ETLW	16	16	C	124	EE
ETLW	16	16	C	156	EE
ETLW	16	16	C	199	EE

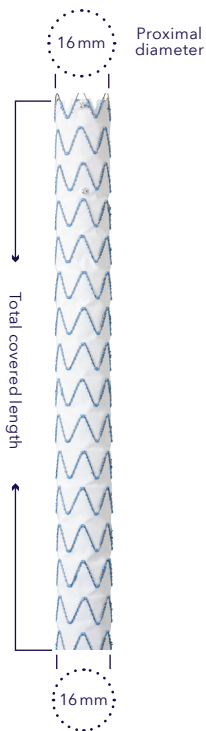

Straight limbs

Endurant™ II/IIs

Stent Graft System

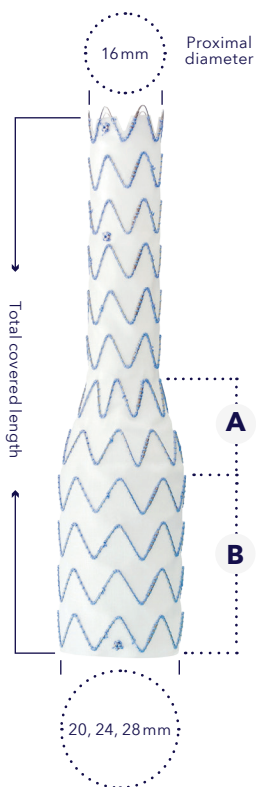

Flared limbs



Flared limbs


	Product code					Graft dimensions (mm)	
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system	A	B
	ETLW	16	20	C	82	EE	10
ETLW	16	20	C	93	EE	10	40
ETLW	16	20	C	124	EE	10	40
ETLW	16	20	C	156	EE	10	40
ETLW	16	20	C	199	EE	10	40
ETLW	16	24	C	82	EE	20	30
ETLW	16	24	C	93	EE	20	40
ETLW	16	24	C	124	EE	20	40
ETLW	16	24	C	156	EE	20	40
ETLW	16	24	C	199	EE	20	40
ETLW	16	28	C	82	EE	20	30
ETLW	16	28	C	93	EE	20	40
ETLW	16	28	C	124	EE	20	40
ETLW	16	28	C	156	EE	20	40
ETLW	16	28	C	199	EE	20	40

Endurant™ II/IIIs

Stent Graft System

Iliac extensions

Product code					
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system
ETEW	10	10	C	82	EE
ETEW	13	13	C	82	EE
ETEW	20	20	C	82	EE
ETEW	24	24	C	82	EE
ETEW	28	28	C	82	EE

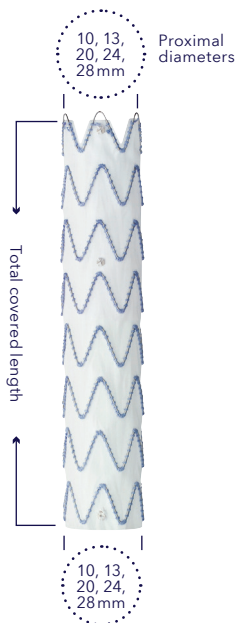


Iliac extensions



AUI


	Product code					Graft dimensions (mm)	
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system	A	B
ETUF	23	14	C	102	EE	30	40
ETUF	25	14	C	102	EE	30	40
ETUF	28	14	C	102	EE	30	40
ETUF	32	14	C	102	EE	30	40
ETUF	36	14	C	102	EE	30	40

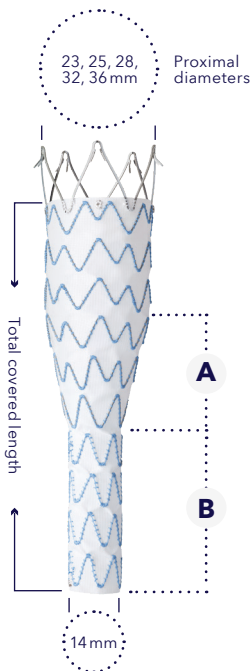

Endurant™ II AUI

Endurant™ II/IIa

Stent Graft System

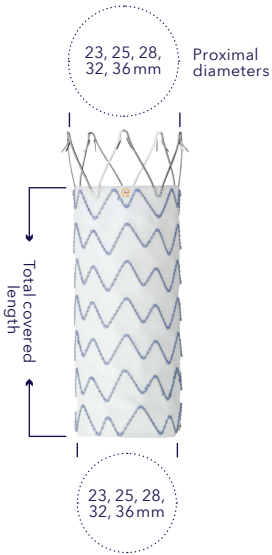

Aortic extensions



Aortic extensions

	Product code				
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Total covered length (mm)	Delivery system
ETCF	23	23	C	49	EE
ETCF	25	25	C	49	EE
ETCF	28	28	C	49	EE
ETCF	32	32	C	49	EE
ETCF	36	36	C	49	EE
ETTF	23	23	C	70	EE
ETTF	25	25	C	70	EE
ETTF	28	28	C	70	EE
ETTF	32	32	C	70	EE
ETTF	36	36	C	70	EE

Valiant™ Stent Graft

with Captivia™ Delivery System

Deploy durability

Precise deployment†

- Easy three step deployment process†
- Tip capture provides controlled deployment and precise placement in the thoracic aorta
- Tip capture release handle provides simple turn-and-pull motion to release proximal stents

Optimal seal†

- Proximal FreeFlo configuration evenly distributes radial force over multiple apices
- Mini support spring optimizes proximal apposition with the vessel wall
- Only device that maintains complete apposition regardless of angulation and oversizing¹

Clinical track record in all descending thoracic aortic pathologies^{2,3}

- 5-year outcomes in TAA, PAU, BTAI and Dissection^{2,3}
- Positive aortic remodeling through 5 years in acute complicated Type B aortic dissection^{2,3}
- Broad selection of proximal and distal components and tapered sizes treats a variety of patients^{2,3}

† Test data on file at Medtronic. Bench test results may not be indicative of clinical performance.


¹ Canaud L, Cathala P, Joyeux F, Branchereau P, Marty-Ané C, Alric P. Improvement in conformability of the latest generation of thoracic stent grafts. *J Vasc Surg.* April 2013;57(4):1084-1089.

² Bavaria J, Brinkman W, Hughes C, et al. Five-year outcomes of endovascular repair of complicated acute type B aortic dissections. *J Thorac Cardiovasc Surg.* 2020; S0022-5223(20)31092-31098.

³ Bavaria J, Brinkman WT, Hueghes GC, et al. Outcomes of Thoracic Endovascular Aortic Repair in Acute Type B Aortic Dissection: Results From the Valiant United States Investigational Device Exemption Study. *Ann Thorac Surg.* September 2015;100(3):802-808.



Component placement guide

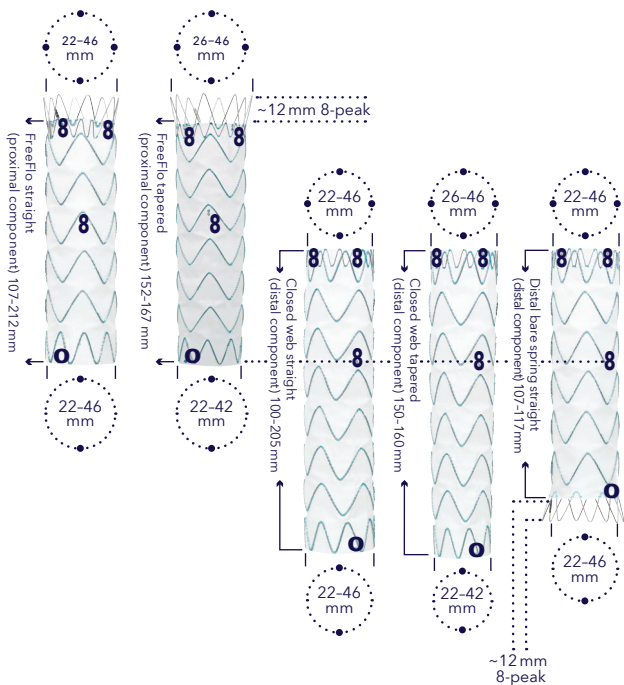

Distinct radiopaque markers

- 8** Figur8 marker
- 0** Zer0 marker

Valiant™ Stent Graft

with Captivia™ Delivery System

Medtronic recommends that the Valiant™ Stent Graft with Captivia™ Delivery System be used according to the sizing guidelines contained in the IFU. Proper sizing of the Valiant™ Stent Graft is the responsibility of the physician.

Aneurysms, penetrating ulcers and traumatic ruptures:

Full sizing guidelines are detailed in the *Instructions for Use* (IFU). Additional oversizing should not be incorporated. Please visit manuals.medtronic.com for more detailed sizing information.

Dissection:

For Dissections, appropriate oversizing has already been incorporated into the recommended sizes. Additional oversizing should not be incorporated. Oversizing of the stent graft to the vessel >10% may be unsafe in the presence of dissecting tissue or intramural hematoma.

For additional sections:

When multiple stent grafts are needed to exclude the target lesion, and the component junction or overlapping connection is not supported by the aorta, the diameter of the inside component should be oversized by 4 mm relative to the outside component. If it is supported by the vessel, oversizing to the supporting native vessel should be used.

Fusiform & saccular aneurysms and penetrating ulcers sizing guidelines

Native vessel (mm)	Suggested FreeFlo straight stent graft diameter (mm)
18, 19	22
20, 21	24
22, 23	26
24, 25	28
25, 26, 27	30
27, 28, 29	32
29, 30, 31	34
31, 32	36
33, 34	38
35, 36	40
37, 38	42
39, 40	44
41, 42	46



Blunt traumatic aortic injury sizing guidelines

Native vessel (mm)	Suggested stent graft diameter (mm)
18	22
19	22
20	22
21	22
22	24
23	24
24	26
25	26
26	28
27	28
28	30
29	32
30	32
31	34
32	34
33	36
34	36
35	38
36	38
37	40
38	40
39	42
40	42
40	44
41	44
42	44
42	46
43	46
44	46


Dissection sizing guidelines

Native vessel (mm)	Suggested stent graft diameter (mm)
20	22
21	22
22	24
23	24
24	26
25	26
26	28
27	28
28	30
29	32
30	32
31	34
32	34
33	36
34	36
35	38
36	38
37	40
38	40
39	42
40	42
40	44
41	44
42	44
42	46
43	46
44	46

Valiant™ Stent Graft

with Captivia™ Delivery System

Valiant™ Captivia™ thoracic stent graft system product code description

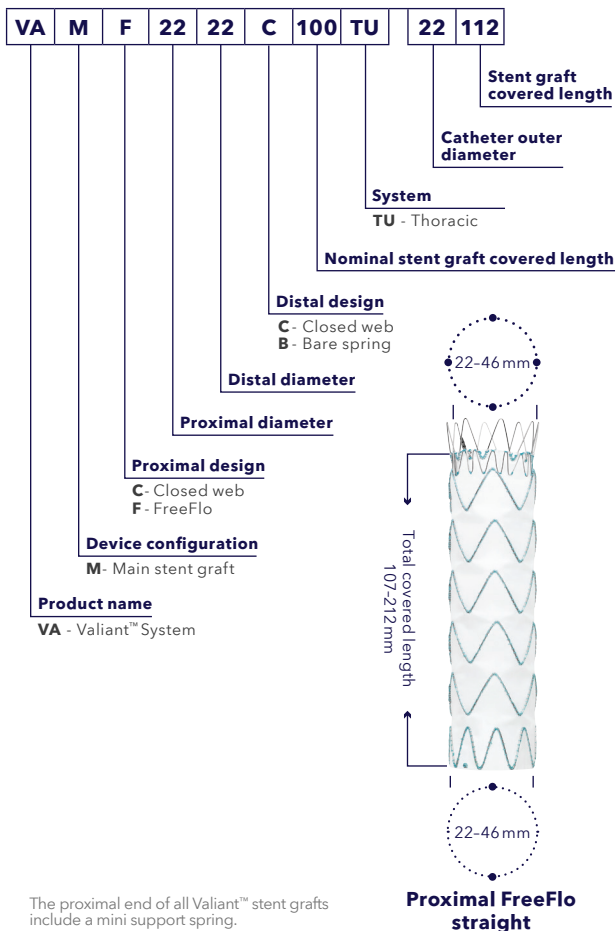

The proximal end of all Valiant™ stent grafts include a mini support spring.



Proximal FreeFlo straight

Product code						Catheter outer diameter (Fr)	Stent graft covered length (mm)
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design				
VAMF	22	22	C	100	TU	22	112
VAMF	24	24	C	100	TU	22	112
VAMF	26	26	C	100	TU	22	112
VAMF	28	28	C	100	TU	22	117
VAMF	30	30	C	100	TU	22	117
VAMF	32	32	C	100	TU	22	117
VAMF	34	34	C	100	TU	24	107
VAMF	36	36	C	100	TU	24	107
VAMF	38	38	C	100	TU	24	107
VAMF	40	40	C	100	TU	24	107
VAMF	42	42	C	100	TU	25	112
VAMF	44	44	C	100	TU	25	112
VAMF	46	46	C	100	TU	25	112
VAMF	22	22	C	150	TU	22	152
VAMF	24	24	C	150	TU	22	152
VAMF	26	26	C	150	TU	22	152
VAMF	28	28	C	150	TU	22	157
VAMF	30	30	C	150	TU	22	157
VAMF	32	32	C	150	TU	22	157
VAMF	34	34	C	150	TU	24	167
VAMF	36	36	C	150	TU	24	167
VAMF	38	38	C	150	TU	24	167
VAMF	40	40	C	150	TU	24	167
VAMF	42	42	C	150	TU	25	157
VAMF	44	44	C	150	TU	25	157
VAMF	46	46	C	150	TU	25	162
VAMF	30	30	C	200	TU	22	192
VAMF	32	32	C	200	TU	22	192
VAMF	34	34	C	200	TU	24	212
VAMF	36	36	C	200	TU	24	207
VAMF	38	38	C	200	TU	24	207
VAMF	40	40	C	200	TU	24	212
VAMF	42	42	C	200	TU	25	207
VAMF	44	44	C	200	TU	25	212
VAMF	46	46	C	200	TU	25	212

Valiant™ Stent Graft

with Captivia™ Delivery System



**Proximal FreeFlo
tapered**



Proximal FreeFlo tapered

Product code							
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Nominal stent graft covered length (mm)		Catheter outer diameter (Fr)	Stent graft covered length (mm)
VAMF	26	22	C	150	TU	22	152
VAMF	28	24	C	150	TU	22	157
VAMF	30	26	C	150	TU	22	157
VAMF	32	28	C	150	TU	22	157
VAMF	34	30	C	150	TU	24	167
VAMF	36	32	C	150	TU	24	167
VAMF	38	34	C	150	TU	24	167
VAMF	40	36	C	150	TU	24	167
VAMF	42	38	C	150	TU	25	157
VAMF	44	40	C	150	TU	25	157
VAMF	46	42	C	150	TU	25	162

Valiant™ Stent Graft

with Captivia™ Delivery System



Closed web straight



Closed web straight

Product code						Catheter outer diameter (Fr)	Stent graft covered length (mm)
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design				
VAMC	22	22	C	100	TU	22	105
VAMC	24	24	C	100	TU	22	105
VAMC	26	26	C	100	TU	22	105
VAMC	28	28	C	100	TU	22	110
VAMC	30	30	C	100	TU	22	110
VAMC	32	32	C	100	TU	22	110
VAMC	34	34	C	100	TU	24	100
VAMC	36	36	C	100	TU	24	100
VAMC	38	38	C	100	TU	24	100
VAMC	40	40	C	100	TU	24	100
VAMC	42	42	C	100	TU	25	105
VAMC	44	44	C	100	TU	25	105
VAMC	46	46	C	100	TU	25	105
VAMC	22	22	C	150	TU	22	145
VAMC	24	24	C	150	TU	22	145
VAMC	26	26	C	150	TU	22	145
VAMC	28	28	C	150	TU	22	150
VAMC	30	30	C	150	TU	22	150
VAMC	32	32	C	150	TU	22	150
VAMC	34	34	C	150	TU	24	160
VAMC	36	36	C	150	TU	24	160
VAMC	38	38	C	150	TU	24	160
VAMC	40	40	C	150	TU	24	160
VAMC	42	42	C	150	TU	25	150
VAMC	44	44	C	150	TU	25	150
VAMC	46	46	C	150	TU	25	155
VAMC	30	30	C	200	TU	22	185
VAMC	32	32	C	200	TU	22	185
VAMC	34	34	C	200	TU	24	205
VAMC	36	36	C	200	TU	24	200
VAMC	38	38	C	200	TU	24	200
VAMC	40	40	C	200	TU	24	205
VAMC	42	42	C	200	TU	25	200
VAMC	44	44	C	200	TU	25	205
VAMC	46	46	C	200	TU	25	205

Valiant™ Stent Graft

with Captivia™ Delivery System



Closed web tapered



Closed web tapered

Product code							
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Nominal stent graft covered length (mm)		Catheter outer diameter (Fr)	Stent graft covered length (mm)
VAMC	26	22	C	150	TU	22	150
VAMC	28	24	C	150	TU	22	150
VAMC	30	26	C	150	TU	22	150
VAMC	32	28	C	150	TU	22	150
VAMC	34	30	C	150	TU	24	160
VAMC	36	32	C	150	TU	24	160
VAMC	38	34	C	150	TU	24	160
VAMC	40	36	C	150	TU	24	160
VAMC	42	38	C	150	TU	25	150
VAMC	44	40	C	150	TU	25	150
VAMC	46	42	C	150	TU	25	155

Valiant™ Stent Graft

with Captivia™ Delivery System



Distal bare spring straight



Distal bare spring straight

Product code							
	Proximal graft diameter (mm)	Distal graft diameter (mm)	Distal design	Nominal stent graft covered length (mm)		Catheter outer diameter (Fr)	Stent graft covered length (mm)
VAMC	22	22	B	100	TU	22	112
VAMC	24	24	B	100	TU	22	112
VAMC	26	26	B	100	TU	22	112
VAMC	28	28	B	100	TU	22	117
VAMC	30	30	B	100	TU	22	117
VAMC	32	32	B	100	TU	22	117
VAMC	34	34	B	100	TU	24	107
VAMC	36	36	B	100	TU	24	107
VAMC	38	38	B	100	TU	24	107
VAMC	40	40	B	100	TU	24	107
VAMC	42	42	B	100	TU	25	112
VAMC	44	44	B	100	TU	25	112
VAMC	46	46	B	100	TU	25	112

Features

Reinforced seal, durable outcomes

- EndoSuture Aneurysm Repair (ESAR) with the Heli-FX™ EndoAnchor™ system enhances the durability of EVAR and TEVAR endografts and protects against neck dilatation.¹
- EndoAnchor™ implants are designed to provide radial support via transmural fixation, offering the strength and stability of a surgical anastomosis in an endovascular fashion²
- The EndoAnchor™ implant and Heli-FX™ EndoAnchor™ system have been evaluated via in vitro testing.

Expanding patient care options

- Endurant™ II/IIIs stent graft system and Heli-FX™ EndoAnchor™ system
- The first off-the-shelf short neck EVAR solution
- Endurant II/IIIs stent graft system is indicated for proximal neck length of ≥ 4 mm and < 10 mm when used in conjunction with the Heli-FX EndoAnchor system.


EVAR ordering information

AAA components (mm)	Deflected tip reach (mm)	Recommended neck diameter (mm)	Working length (cm)	O.D. (Fr)	Catalog number
Heli-FX™ system guide, 22	22	18-28	62	16	SG-64
Heli-FX™ system guide, 28	28	28-32	62	16	HG-16-62-28
Heli-FX™ applier and EndoAnchor™ cassette (w/10 EndoAnchor™ implants)	NA	NA	86	12	SA-85
Ancillary EndoAnchor™ cassette (w/5 EndoAnchor™ implants)	NA	NA	NA	NA	EC-05

* Third party brands are trademarks of their respective owners

¹ Tassiopoulos AK, Monastiriotes S, Jordan WD, Muhs BE, Ouriel K, De Vries JP. Predictors of early aortic neck dilatation after endovascular aneurysm repair with EndoAnchors. *J Vasc Surg.* July 2017;66(1):45-52.

² Melas N, Perdikides T, Saratzis A, et al. Helical EndoStaples enhance endograft fixation in an experimental model using human cadaveric aortas. *J Vasc Surg.* 2012 Jun;55(6):1726-33.



TEVAR ordering information

TAA components (mm)	Deflected tip reach (mm)	Recommended neck diameter (mm)	Working length (cm)	O.D. (Fr)	Catalog number
Heli-FX™ system guide, 22	22	18-28	90	18	HG-18-90-22
Heli-FX™ system guide, 32	32	28-38	90	18	HG-18-90-32
Heli-FX™ system guide, 42	42	38-42	90	18	HG-18-90-42
Heli-FX™ applicator and EndoAnchor™ cassette (w/10 EndoAnchor™ implants)	NA	NA	114cm	12	HA-18-114
Ancillary EndoAnchor™ cassette (w/5 EndoAnchor™ implants)	NA	NA	NA	NA	EC-05

Steerant™

Super Stiff Guidewire

It's just right

Meet Steerant, the aortic guidewire designed just right for your aortic procedures. The guidewire's soft, atraumatic tip gradually transitions to a stiff main body, providing protection for fragile aortic anatomy along with the support needed for device deployment. Steerant guidewire is offered in lengths tailored for EVAR and TEVAR procedures.

Tailored for aortic procedures

- Lengths and tip curves designed for EVAR and TEVAR
- The 8 cm radiopaque tip facilitates clear guidewire navigation and target visualization

Balanced control


- Right balance of stiffness and trackability
- Gradual stiffness transition provides balanced control in straightforward and challenging anatomy
- PTFE coating provides smooth device delivery


Protects fragile aortic anatomy

- Flexible, soft tip provides an atraumatic interface
- 15 cm flexible tip to protect anatomy

Right length.
Right stiffness.
Right control.

It's just right.

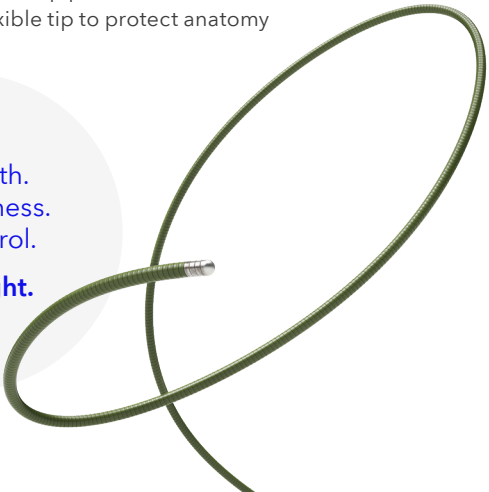

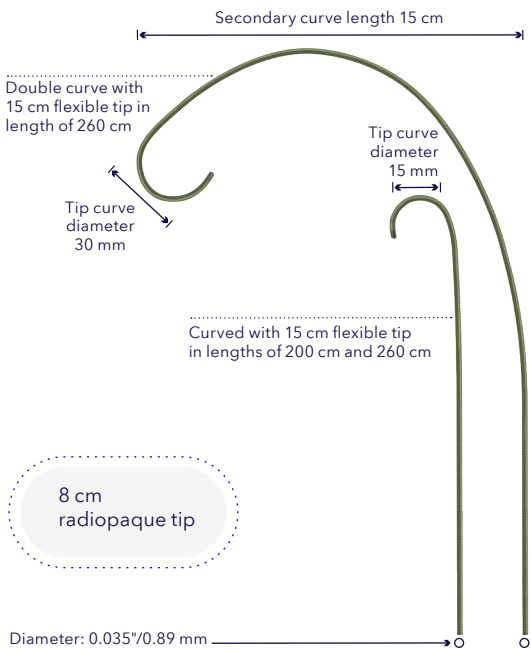

Ordering information

Catalog number	Length (cm)	Tip shape	Transition length (cm)	Tip curve diameter (mm)	Secondary curve length (cm)	Wire diameter (in/mm)	RO length (cm)
AGWSJ200	200	Curved	15	15	N/A	0.035/0.89	8
AGWSJ260	260	Curved	15	15	N/A	0.035/0.89	8
AGWDJ260	260	Double curve	15	30	15	0.035/0.89	8

Sentrant™


Introducer Sheath with Hydrophilic Coating

Features

Engineered to deliver procedural confidence

- EnsureSeal technology delivers superior leak resistance versus competitors†
- Coil-reinforced tubing for added stability and kink resistance
- Maintains lubricity after multiple insertions
- Radiopaque dilator shaft and sheath tip for accurate visualization and guidance
- 64 cm configuration launched to service a broader range of anatomies and procedures
- Compatible with a wide range of endovascular portfolios


Leak resistance versus Cook Check-Flo Performer™* introducer sheath and Gore DrySeal™* Flex introducer sheath†

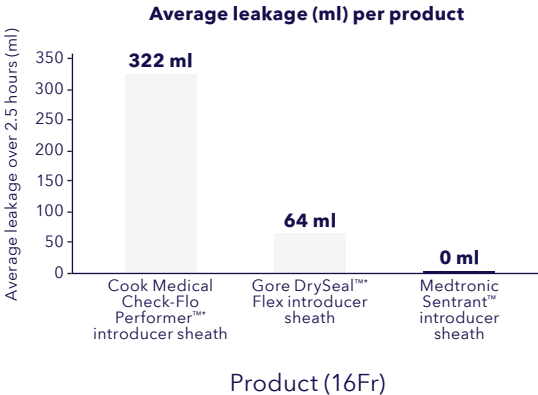

* Third party brands are trademarks of their respective owners

† Leak Resistance Bench Test Data on file at Medtronic. Test data not indicative of clinical performance. Bench Test compared Cook Check-Flo Performer™* 16 Fr and Gore DrySeal™* Flex 16 Fr to Sentrant™ 16 Fr. Graph shows average leakage over an extrapolated 2.5 hour procedure.

The choice for hemostasis†

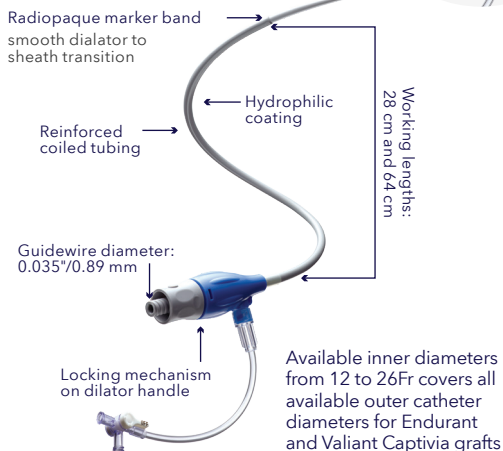

Ordering information

Catalog number	Inner diameter (Fr)	Usable length (cm)
SENSH1228W	12	28
SENSH1428W	14	28
SENSH1628W	16	28
SENSH1828W	18	28
SENSH2028W	20	28
SENSH2228W	22	28
SENSH2428W	24	28
SENSH2628W	26	28
SENSH1264W	12	64
SENSH1464W	14	64
SENSH1664W	16	64
SENSH1864W	18	64
SENSH2064W	20	64
SENSH2264W	22	64
SENSH2464W	24	64
SENSH2664W	26	64

† Leak Resistance Bench Test Data on file at Medtronic. Test data not indicative of clinical performance. Bench Test compared Cook Check-Flo Performer™ 16 Fr and Gore DrySeal™ Flex 16 Fr to Sentrant™ 16 Fr. Graph shows average leakage over an extrapolated 2.5 hour procedure.

Reliant™

Stent-Graft Balloon Catheter

Features

Expand possibilities

A single-solution balloon catheter for your stent graft procedure needs

Clinical uses include:

- Abdominal and thoracic use
- Endograft modeling
- Endoleak sealing support

Wide range of balloon inflation diameters

Balloon inflation table

46 mm balloon	
Diameter (mm)	MI (cc)
10	3
20	9
30	19
40	41
46 [†]	60

Caution: This table is only a guide. Balloon expansion should be carefully monitored under fluoroscopy. Do not exceed maximum inflation diameter (46 mm). Rupture of balloon may occur.

Product information

Reliant™ stent graft balloon catheter**

Product code	Inflation diameter (mm)	Shaft size (Fr)	Usable length (cm)	Sheath compatibility (Fr)
AB46	10-46	8	100	12


Please reference appropriate product *Instructions for Use* for a more detailed list of indications, warnings, precautions and potential adverse events.

[†]Maximum inflation diameter.

**Does not contain latex.



Multiple purposes, single solution

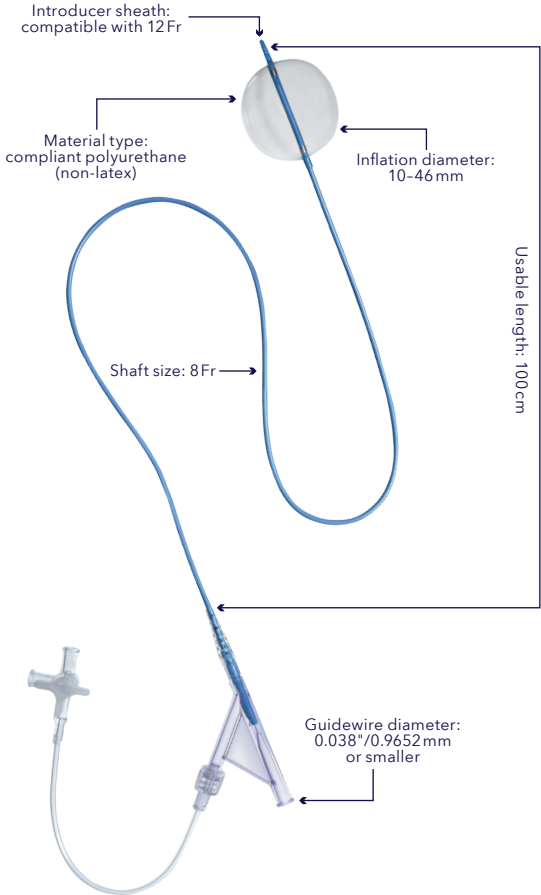

For a listing of indications, contraindications, precautions, warnings, and potential adverse events, please refer to the Instructions for Use.

Medtronic

[medtronic.ca](https://www.medtronic.ca)

©2025 Medtronic. All rights reserved. Medtronic, Medtronic logo and Engineering the extraordinary are trademarks of Medtronic. TM*Third party brands are trademarks of their respective owners. All other brands are trademarks of a Medtronic company.
UC202209954EC CA-CTL-0310c-E Rev. 08/2025